



Neurophone®

Strobel / Service / Vertrieb



Manual

Flanagan Neurophone NF3

Contents, Guarantee

- 3 The Neurophone – the meditation tool
- 4 Scope Of Delivery
- 5 Function, Operations
- 6 - 7 Sound-Transducer
 - Hearing Test
 - Palm feeling test for sensitive people
 - Tip of the tongue test
- Audio Playing
 - Volume Control
- 7 - 9 Handling
 - 9 Utilizing Audio-IN-Signals
 - 10 Connecting Options
 - 11 One NF3 for three!
- 12 Changing The Battery
 - 13 Battery Recommendation
 - 13 Original Flanagan CD
- 14 Pyramid Power
- 15 Pyramid Medal Sensor V
- 16 Contact

Neurophone NF3
with permanent internal noise:
Length x width x height
11.1 x 6.7 x 2.2 cm
incl. alkaline battery 130 g

Battery at delivery
9 V block battery, alkaline, approx. 45 g
standard type 6LR61 or 6F22,
typical capacity 500 to 600 mAh

Sound-Transducer
with 2 stainless steel membranes, 27 mm²,
19 g

One year guarantee
on Flanagan Neurophone NF3

No guarantee on flexible leads,
battery, sound-transducer, adapters.

No guarantee with damage from
mechanical influences and liquids,
including perspiration.

With your Flanagan NF3 Neurophone
you will gain new life awareness,
improve meditation, relaxation,
learning and memory!

The Neurophone – the meditation tool...

... for your electromagnetic awareness and vital energy.

With the **Neurophone**, you can activate all your body cells in a finely tuned way through electromechanical transmitted ultrasonic oscillations. In this way you gain new life awareness, increase your meditation success, improve relaxation, learning and memory. People have reported positive effects after using the **Flanagan Neurophone** on a daily basis, in the morning, before going to sleep, all night or all day.



Dr. G. Patrick Flanagan

Dr. G. Patrick Flanagan has developed his **Neurophones** to perfection.

Patrick was able to prove that the intelligence quotient (IQ) would be significantly increased, due to the synchronization of the brain hemispheres.

Dr. Batteau, who lectured as a researcher at the Tufts University in Boston, invited the 21 year-old Patrick Flanagan with his Neurophone invention, to a research project on the communication between humans and dolphins.


The subdued ultrasonic sound of **Flanagan's Neurophones** is received by the sacculle in the inner ear. The sacculle is the organ of balance and gravity.

With **Original Flanagan Neurophones** you can reduce nervousness and stress, both during sleep or when awake and get rid of "electrostress". This can result in a preventive benefit for your vital energy and health.

Superlearning: In 1971 the Bulgarian physician Dr. Georgi Lozanov propagandized the system of suggestopaedia for faster learning. For your personal **Superlearning** you can balance your brainwave spectrum by help of a Neurophone for your boosted learning effect.

The status of the Delta-, Theta-, Alpha- and Beta-frequencies in the band of 0.5 to 3.5 Hz can be analyzed by an EEG (electroencephalography).

Scope Of Delivery

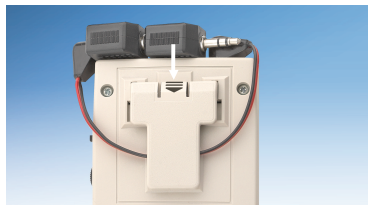

NF3 Neurophone with adapters

Neurophone NF3 with releasable clip and 9 Volt battery (inside battery box)



2 sound-transducer for meditation

each with 2 membranes of stainless steel;
flat ribbon cable, approx. 1200 mm;
angled phone jack 3.5 mm;
sliding sleeve, approx. 12 mm;
Velcro tape, approx. 110 x 16 mm.



The wooden stick is very important!

Adapters and wooden stick

- 1 Adapter cable for connecting the IN jack to an audio jack.
- 2 adapters (splitters), phone jack 3.5 mm and double jack 3.5 mm as standard part.
- 1 Wooden stick, 28 mm x 4 mm° (inside battery box):
 - spacer between wall and plug
 - for releasing the battery plug
 - for adjusting the output voltage

1 Patrick Flanagan CD with sound of flowing water and affirmations in German and English



CD with affirmations

Function, Operations


Function

The output signal with adjustable volume and voltage from 5 to 20 V has a constant oscillation of approx. 40 kHz (this frequency is ultrasonic). In all operational modes, the output signal contains **internal noise**, even when the volume is at minimum. This alterable internal noise interacts with you as well as with changes in your settings or influences from surroundings and can even become quieter with higher output voltage.

The possibility of coupling with audio-(IN)-signals (e.g. for learning purposes, relaxation and sleeping-aid under noise exposure) can reinforce the benefit.

The internal noise and audio-(IN)-signals also become acoustically audible by ultrasonically induced resonance.

ON/OFF, volume, light emitting diode (LED)

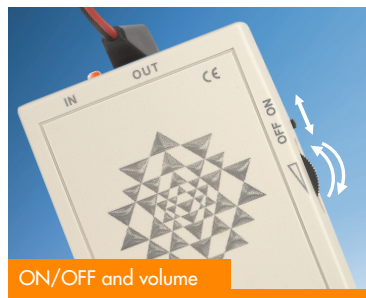


ON/OFF and volume

Light Emitting Diode (LED)

The light signal serves as a power indicator of the brightness changing upon the battery reserve. The decrease in brightness becomes noticeable at approx. 4 volts.

Volume adjustment:

Three visible lengths on the setting dial:
 $3 \times 90^\circ = 270^\circ$ without switching function!

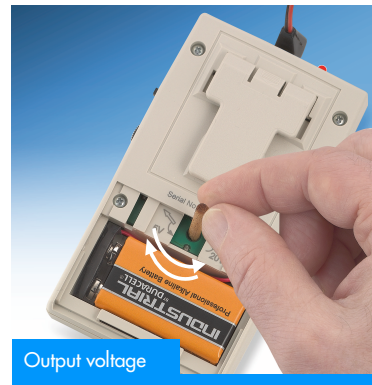

Output voltage

Increasing counterclockwise causes IN-signals to be heard louder. At 5 V (minimum) plus a new alkaline battery the NF3 can operate for up to 50 hours. Higher voltage leads to proportionally higher power consumption.

Sound-Transducer

The membranes are electromechanically made to oscillate. The amplitude is in micrometers.

Even at minimum volume and voltage the physiological impact remains fully efficient.

Audio Playing

Push the phone jack of the sound-transducer as far as it will go (!) into the OUT jack. Using the adapter cable (a 3.5 phone jack at each end) connect the 'IN' jack to the headphone jack of your individual player.




For large audio players with a 6.3 mm jack there are standard adapters for reducing a 6.3 mm format to 3.5 mm.

Hearing Test

ON, max. volume, voltage = 5 V, plug in OUT: Hold both membranes touching metal to metal and press one Velcro tape side onto an ear canal. For the very first detection of the internal noise a briefly hearing test can be done by a headphone's left speaker when the headphone is connected in the OUT jack.

Volume Control

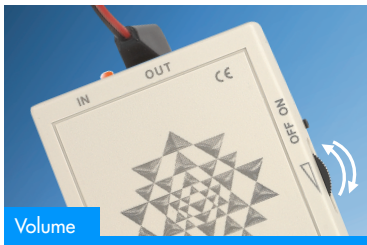

Maximum is recommended for the hearing test. Standard operation with internal noise only even at volume's minimum.

IN-signals become perceptible from half a dial length above minimum limit.

The volume adjustment has very little effect on power consumption.

Because of permanent internal noise the NF3 serves 100% physiological effect on volume-minimum and without audio-(IN)-signal.

Palm feeling test for sensitive people

ON, min. volume, voltage = 5 V:

The unit already produces the full effects. Energy-sensitive subjects can feel warmth, coolness and / or tingling, also a rising or sinking energy, when placing the palm of their hand above one membrane (no touching) and moving it up and down very slowly.

Handling

Most popular and safe to place the NF3 is in the belly's area inside the waistband of your pants or skirt, with the NF3 front side facing the body. The attachment clip is then on the outside of your waistband. In this way there is no danger for breaking the clip or NF3 falling off when bending over. An alternative would be a carrying bag.



Tip of the tongue test

ON, max. volume, voltage = 20 V:

Placing a thumb onto one of the membranes and the tip of the tongue with an area of approx. 1 x 1 mm onto the other membrane produces an enormous feeling of vibration which disappears immediately if the tongue is pressed more firmly.



Placing the membranes

The optimal position and distance between them results from the goal and experience.



Use the sliding sleeve if required, e.g. before overnight sleeping, for stretching as loosely as possible.

The best perception of audio signals is obtained, positioning the sound-transducer on the forehead for increased skin contact.

Attachment aids: Velcro tape, headband, plaster, cap, helmet etc.

Common Recommendations:

The membranes can also be asymmetrically placed for skin contact from head to toe. A minimum skin contact is already sufficient for all of the physiological effects.

Safe positions: head, neck, shoulder



Before attaching the cables, clean all the interested skin areas with a dry cloth.

The cables may not have twists, kinks or bends!

It requires several days use of Neurophone in order to develop an experience of awareness. The unit can be used without or with an audio-(IN)-signal for 60 minutes or longer, while carrying out an activity, resting, or even when asleep.


Be guided by your own intuition as to how long you use the device. Position the sound-transducer/s also on other parts of your body.

Test your perceptions in normal everyday life as well as in stress and painful situations.

Observe and note down the effects and results of your original Flanagan Neurophone:

on the way for better health / how other people perceive you / before sleeping, during and after sleep, as well as regarding dreams / on your 5 senses / during the day's work / during a car or plane trip / during musical activity / during physical activities, sports, fine motor demands (e.g. speaking, finger exercising, dancing) / during meditation / during intense stress / when changing behavioral patterns / during lessons, lectures or concerts / when outdoors in nature / when acquiring or remembering knowledge / etc.

Experience an organ's or orchestra's sound whilst one membrane is pressed directly onto the left ear canal and the other one onto the right ear canal at the same time. **Animals and plants can be included in the experimental use.**

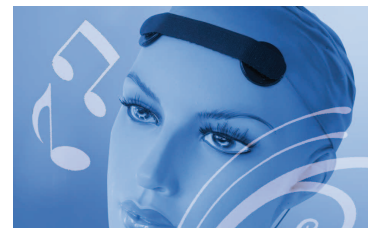

Utilizing Audio-(IN)-Signals

The sound and speech signals played through the NF3 IN can increase spiritual empowerment both consciously and subconsciously, well-being, learning effect and memory.

Playing the provided Original Flanagan CD can also be helpful here.

Options:

1. NF3 with recorded audio signal and parallel audio headphones
2. NF3 with recorded audio signal





Poor quality recordings are a pity. This quality, however, is of secondary importance regarding to a desired effect if you are able to perceive the main signal.

The NF3 transforms the player's stereo signal into a mono signal.

The development of your perceived reality depends on the information that reaches your subconscious mind.

Connecting Options

The possible parallel use of 2 sound-transducers and 2 splitters opens interesting perspectives for one or two users.
The battery load is increased slightly through the 2nd sound-transducer.

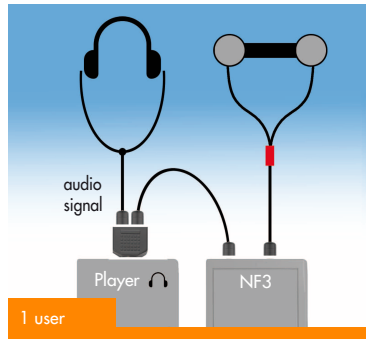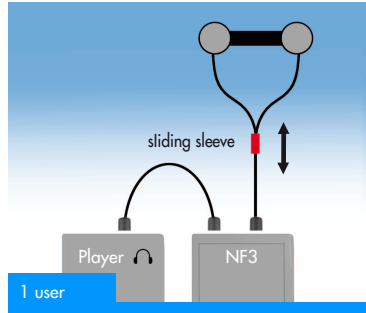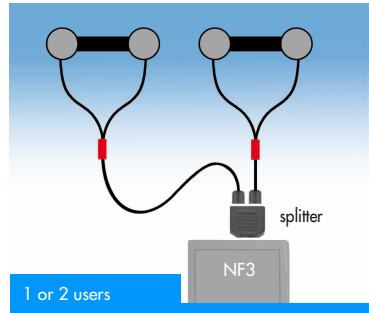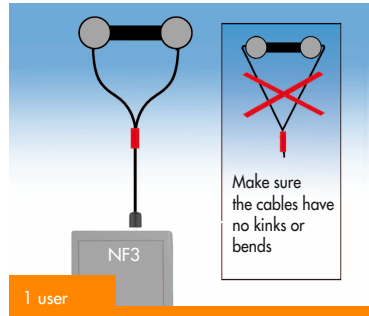

A user circle is formed by two or more people (eventually animals) who touch each other's hands, for example:
Both sound-transducer membranes are included in a similar way like the hands of a user cycle's person.

One NF3 for three!



Changing The Battery



Step 1

Release the battery-plug using the wooden stick by **pressing to the left only**.



Step 2

Turn the Neurophone over and let the battery drop into your hand.

Work on a brand-new battery



Step 3 (if required)

For each new battery expand the ring contact using the opposite contact of a similar battery. This makes connecting to the plug in the battery box easier.



Step 4

Press the new battery on to the plug inside the battery box as shown in the illustration. Put back the wooden stick between the side wall and the battery-plug.

Battery Recommendation

The battery supplied with the NF3 can be used until the brightness of the LED begins to decrease. If the battery has discharged to about 3.5 V, the output signal can become unstable with a squeaky sound. The useful physiological effects of the NF3 still remain.

Non-rechargeable 9 volt batteries (**45 g**) or lithium rechargeable batteries such as the Li-Ion type 500 mAh from CONRAD Electronic (**only 30 g**) are usable as a power source.

The CONRAD rechargeable battery is protected from deep discharge through a switch-off at 5 volts.

Only lithium rechargeable batteries with this so-called PCB (protection circuit board) function may be used.

Recharging the battery

Empty batteries should be recharged in a device recommended by the manufacturer and according to his instructions.

Original Flanagan CD with affirmations

CD with water sounds and affirmations in German and English

The affirmations are embedded 3 times in water sounds for each title. Affirmations (constructive thoughts) can be helpful for you in the acquisition of life habits. This pertains to the deep interconnection of the present state, subconscious causes and new directions of thought. You can also replace the affirmation sentences with sentences spoken yourself. This is recommended by many experts, for example in Louise L. Hay's book „Heal Your Body“. She gives tips for the use of affirmations and says: "If we are prepared to work on ourselves mentally then almost everything is possible."



CD with affirmations

1 Fließendes Wasser	1 Flowing Water
2 Energie	6 Energy
3 Geistiges Wachstum	7 Mental Growth
4 Lernen	8 Learning
5 Gesundheit	9 Health

Pyramid Power

Wearing NF3 and Sensor V at the same time enables synergistic effects.

Pyramid Medal Sensor V



Sensor V

Pyramid Power

Dr. Flanagan's work is in a sphere ranging between high-end technology and metaphysics. As a scientist he continually enters uncharted territory and creates interdisciplinary connections; on the other hand he draws his knowledge and his developments from a well-founded spiritual background.

Some of his central themes are life energy and love energy. Through what he has developed he has already achieved his declared goal of significantly increasing people's quality and length of life. (Katrin Klink)

Dr. Flanagan's bestseller „Pyramid Power“ was published millionfold in the USA in 1975.

Cast bronze, electroplated with silver plus gold in two layers. Diameter: 46 mm, Weight: 30 g



Sensor V – the gift idea

Hanns Martin Strobel, Dipl.-Ing.(FH) / VDE

Ingenieurbüro Strobel
Pfinzingstraße 15
90537 Feucht
DEUTSCHLAND

Telefon: 0049 9128 729 -123, Fax: -125
Email: HMSstrobel@nvc.de
www.neurophone-energy.com



ΦPHISCIENCES

PhiSciences Company, Inc.
271 S. Airport Road
Cottonwood, AZ, 86326
U.S.A.

Telephone: 001 928 634 2668
Fax: 001 928 649 0667
Email: Help@Phisciences.com
www.phisciencences.com

Dr. G. Patrick Flanagan and
Hanns Martin Strobel

wish you helpful experiences
and good use of your
Original Flanagan Neurophone NF3.